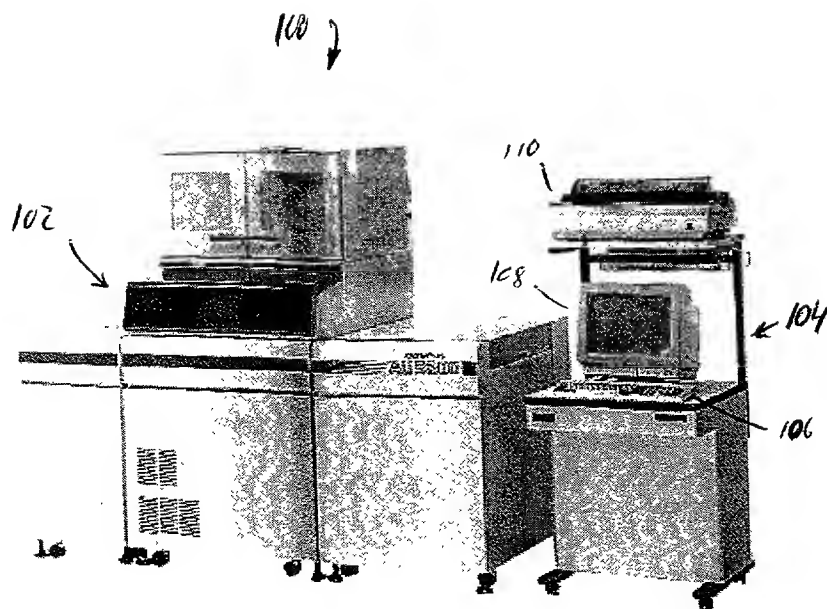


Figure 1



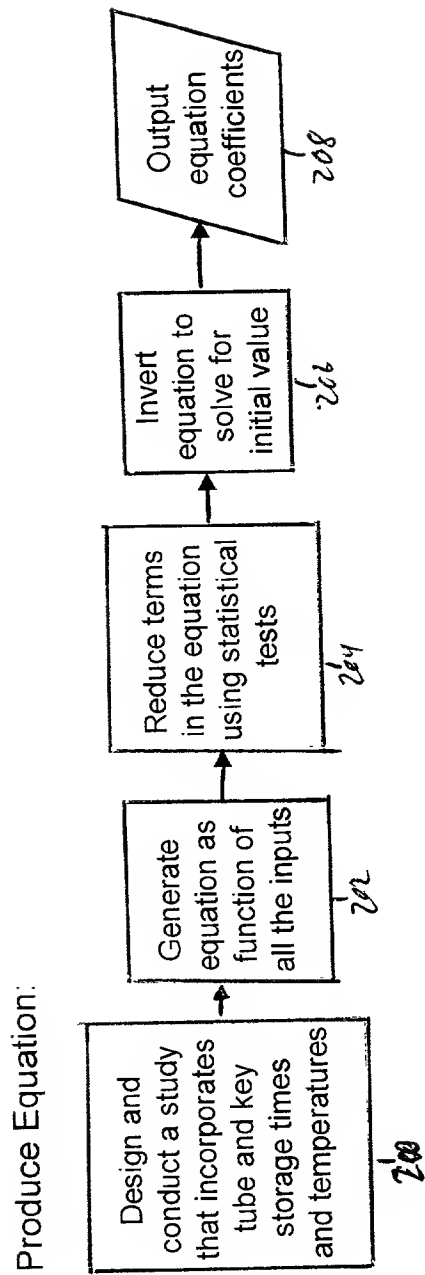


Figure 2

FOOT-1039660

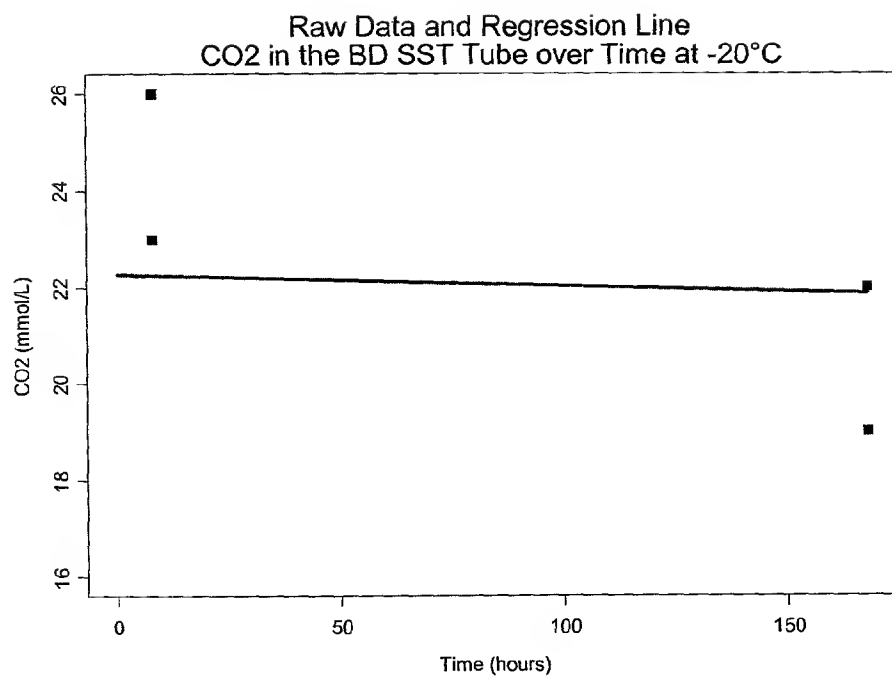


Figure 3(a)

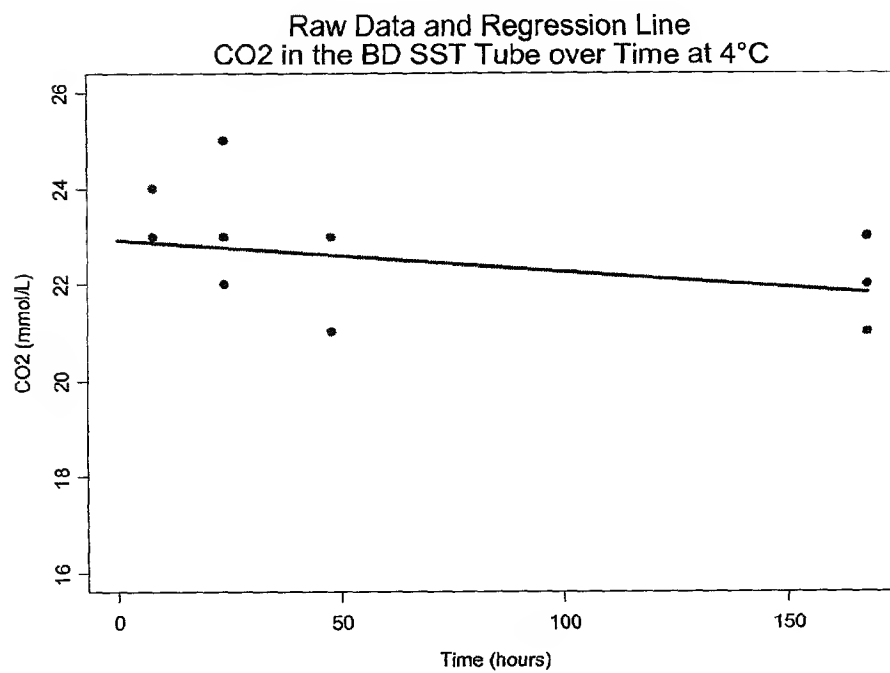


Figure 3(b)

Raw Data and Regression Line
CO₂ in the BD SST Tube over Time at 25°C

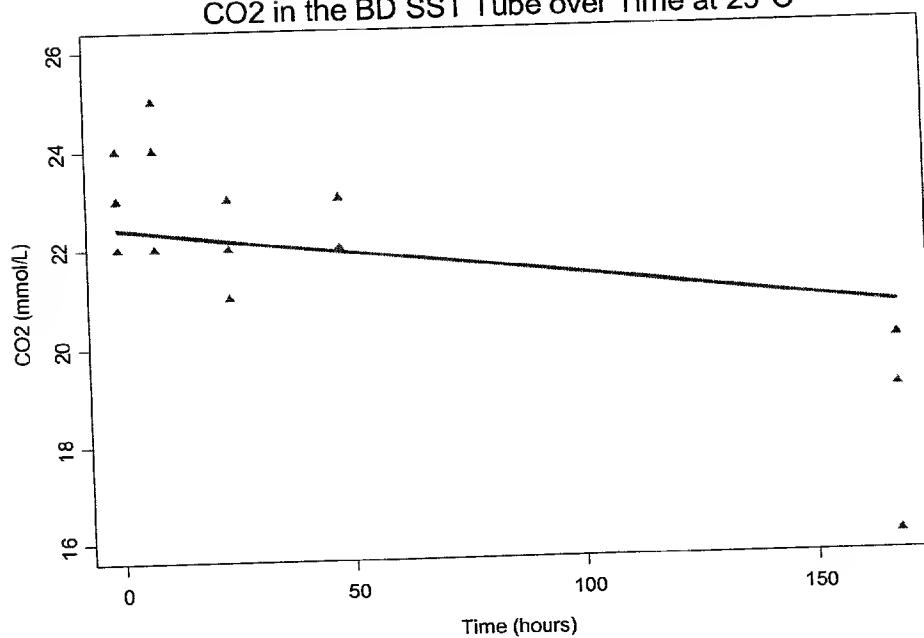


Figure 3(c)

Raw Data and Regression Line
CO₂ in the BD SST Tube over Time at 40°C

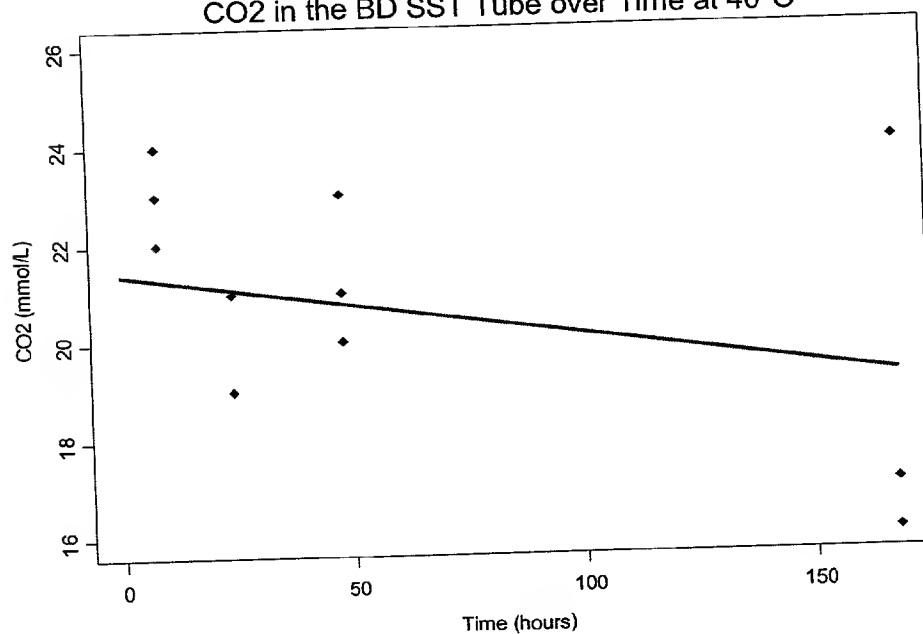


Figure 3(d)

100E11033550

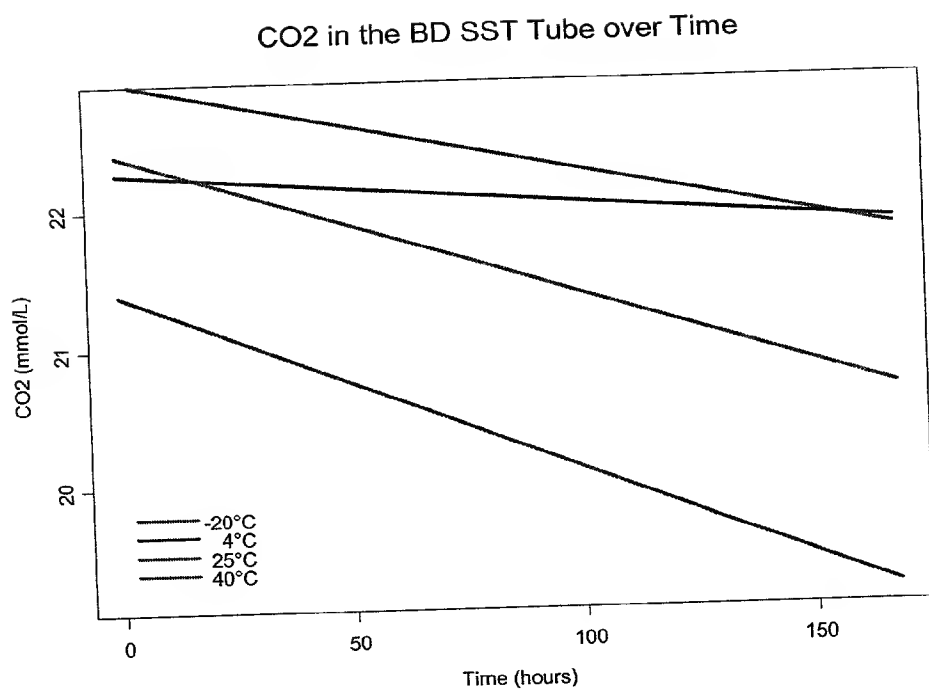


Figure 3(e)

(a)

(b)

(c)

(d)

(e)

(f)

(g)

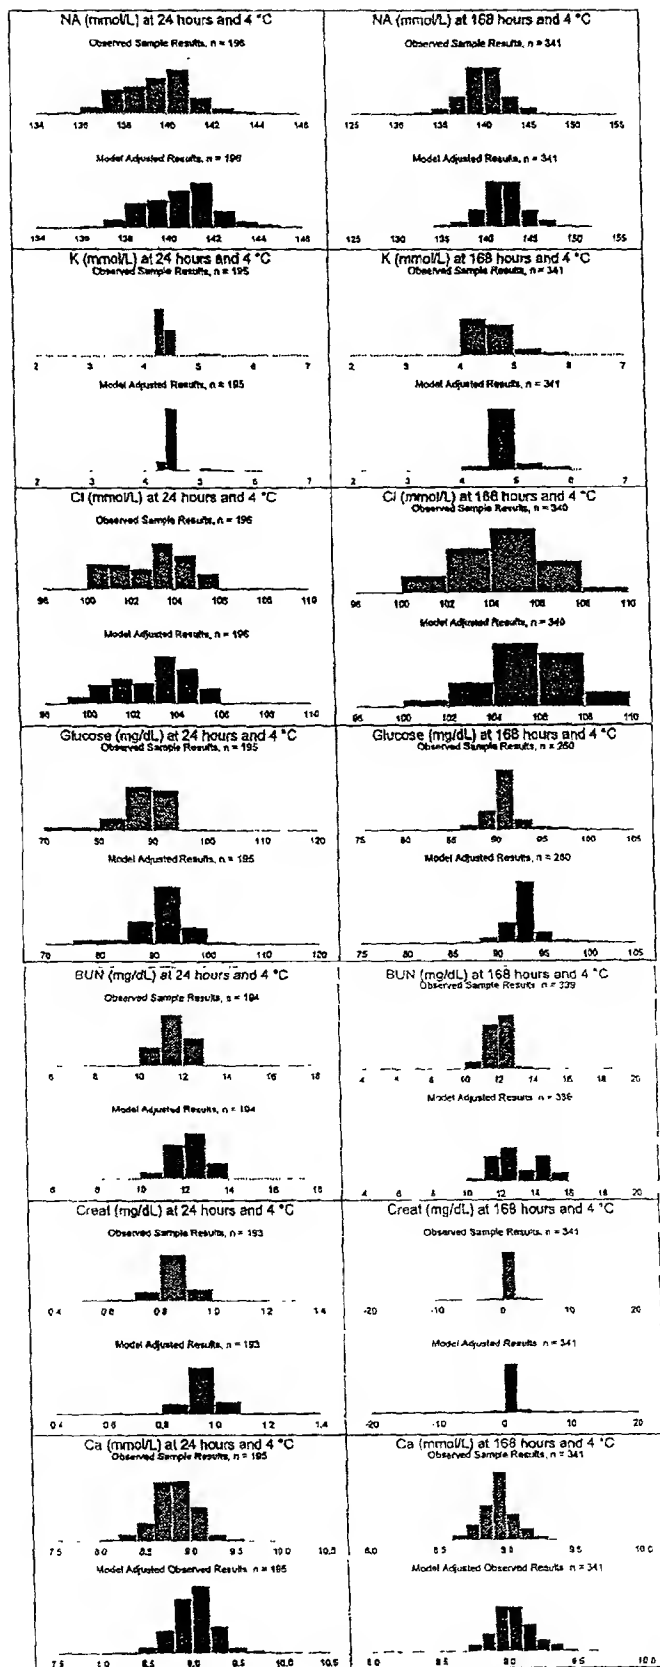


Figure 4

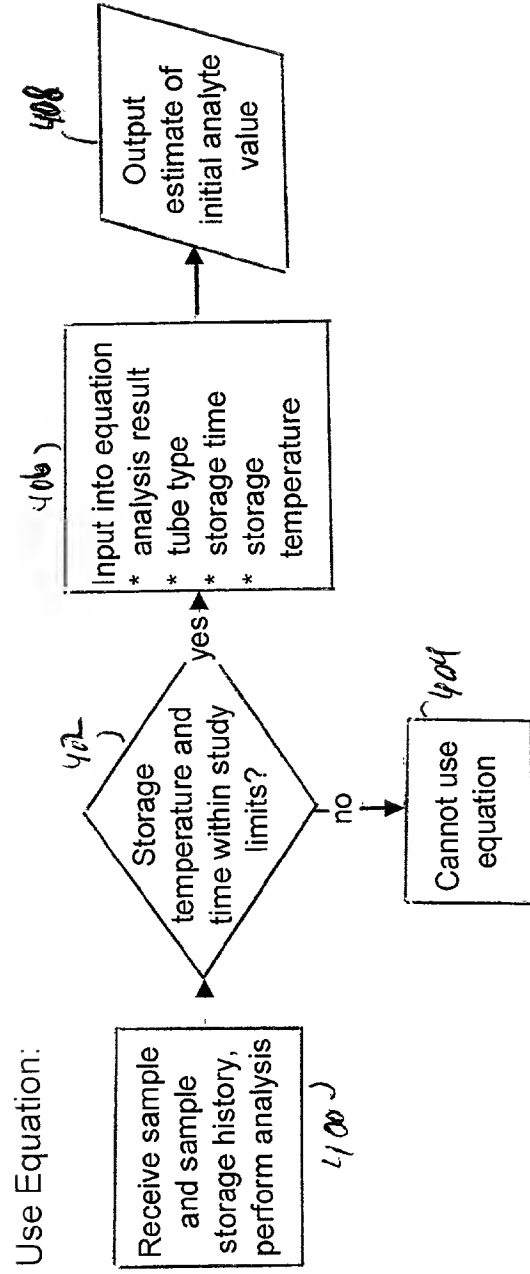


Figure 6